


Instructions for Tamper-Resistant Neckband Removal

To remove the tamper-resistant neckband from the bottle, use one of two methods:

Method 1

- A** Locate the two perforated lines on the tamper-resistant neckband at the top of the bottle cap.

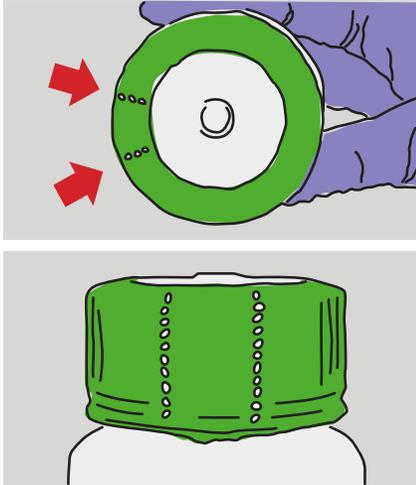

- B** Grasp the portion of the neckband between the two perforated lines and tear in a downward motion.



- C** Remove all pieces of the tamper-resistant neckband from the bottle and discard them.




See reverse side for further instruction →

Method 2

- A** Hold the bottle in one hand and the cap in the other.






- B** Grasp the tamper-resistant neckband material.

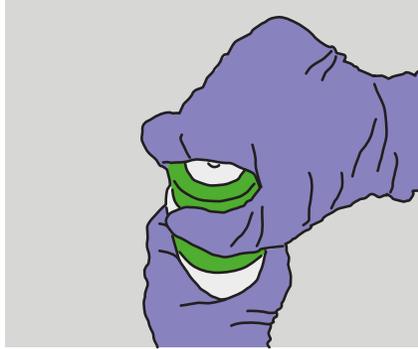

- C** Twist it upward in a clockwise direction to remove the neckband.



Be sure to remove and discard the entire neckband. Do not place the neckband back on the cap once it has been removed. Do not leave any pieces of the neckband remaining on the bottle or the cap.

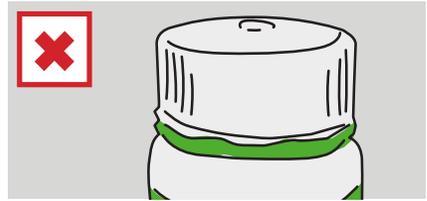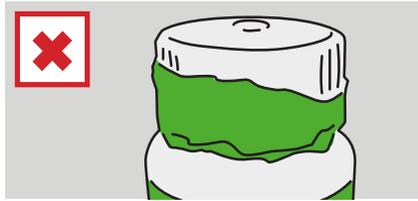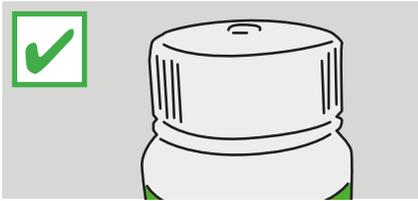

To learn more about ProLacta's tamper-resistant neckbands, please visit www.prolacta.com/neckband or contact your Clinical Sales Specialist.